



# Implant system

**IPX - ICI**  
Internal Connection



Just one **connection**, multiple **possibilities**



Our dental implants are made of **Grade IV Titanium**. They have an **11° conical internal connection** and **unique prosthetic platform**.





Macroscopic implant design that favors great primary stability in any situation.

DIAMETER					
	Ø 3,5 mm	Ø 4 mm	Ø 4,5 mm	Ø 5 mm	
LENGTH	6 mm	-----	Ref. IPX 4006	Ref. IPX 4506	Ref. IPX 5006
	8 mm	Ref. IPX 3508	Ref. IPX 4008	Ref. IPX 4508	Ref. IPX 5008
	10 mm	Ref. IPX 3510	Ref. IPX 4010	Ref. IPX 4510	Ref. IPX 5010
	12 mm	Ref. IPX 3512	Ref. IPX 4012	Ref. IPX 4512	Ref. IPX 5012
	14 mm	Ref. IPX 3514	Ref. IPX 4014	Ref. IPX 4514	-----
	16 mm	Ref. IPX 3516	Ref. IPX 4016	-----	-----
	18 mm	Ref. IPX 3518	Ref. IPX 4018	-----	-----



Macroscopic implant design especially indicated for bone type I and II.

DIAMETER					
Ø 3,2 mm    Ø 3,5 mm    Ø 4 mm    Ø 5 mm					
LENGTH	8 mm	-----	Ref. ICI 03508	Ref. ICI 04008	Ref. ICI 05008
	10 mm	Ref. ICI 03210	Ref. ICI 03510	Ref. ICI 04010	Ref. ICI 05010
	12 mm	Ref. ICI 03212	Ref. ICI 03512	Ref. ICI 04012	Ref. ICI 05012
	14 mm	Ref. ICI 03214	Ref. ICI 03514	Ref. ICI 04014	Ref. ICI 05014

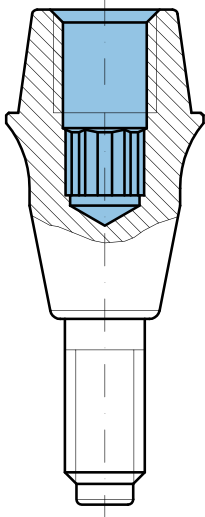

## ***“Simplicity is the ultimate sophistication”***

- ★ Less peri-implant bone loss.
- ★ Fewer mechanical complications.
- ★ Greater torque conservation.
- ★ Crestal bone stability.
- ★ Less micromovements.
- ★ Lower degree of bacterial contamination.





# Transepithelial Multi-unit Aesthetic

## Rotational Prosthetics

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. Indicated for multiple screw-retained prostheses with high aesthetic demands.

### Platform 3,8 mm



#### Multi-unit Aesthetic narrow straight abutment

- 1 mm Ref. MUSR 04010
- 2 mm Ref. MUSR 04020
- 3 mm Ref. MUSR 04030
- 4 mm Ref. MUSR 04040
- 5 mm Ref. MUSR 04050



#### Multi-unit Aesthetic slim straight abutment

- 2 mm Ref. MUSLAR 04020
- 3 mm Ref. MUSLAR 04030
- 4 mm Ref. MUSLAR 04040
- 5 mm Ref. MUSLAR 04050

C€0051

#### Healing cap



Ref. PCT 4030



Ref. PCT 4830

#### Temporary abutment



Ref. PTIMUR 4048

C€0051

#### Impression technique

##### IMPRESSION COPING



Ref. AIPTR 40

##### SCAN-BODY



Ref. SBT MUSR

##### IMPRESSION SCREW



Ref. TAIP 135



Ref. TAIP 200

Laboratory use only

##### ANALOG



Ref. RITR SB 40



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

C€

#### Interfaces

The interfaces can be acquired in package that contains an interface and two **TMU 4048** screws, one clinical and the other for the laboratory.



Ref. PITEMUR 4040



Ref. PGZMUR 40



Ref. PCERCUR 40



Ref. PITEMUR DA4075



Ref. TMU 4048



Ref. TPIA DP4048

C€0051



# Transepithelial Multi-unit Aesthetic

## Rotational Prosthetics

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. Indicated for multiple screw-retained prostheses with high aesthetic requirements in posterior region.

### Platform 4,8 mm



#### Multi-unit Aesthetic wide straight abutment

2 mm	Ref. MUSR 05020
3 mm	Ref. MUSR 05030
4 mm	Ref. MUSR 05040
5 mm	Ref. MUSR 05050

CE0051

### Healing cap



Ref. PCT 5030

CE0051

### Impression technique

Laboratory use only

#### ANALOG



Ref. RITR SB 50



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

#### IMPRESSION COPING



Ref. AIPTR 50

#### SCAN-BODY



Ref. SBT MUSR 50

#### IMPRESSION SCREW



Ref. TAIP 135



Ref. TAIP 200

### Interfaces



Ref. PITEMUR DA5075



Ref. TMU 4048



Ref. TPIA DP4048

CE0051

The interfaces can be acquired in package that contains an interface and two **TMU 4048** screws, one clinical and the other for the laboratory.



# Transepithelial Multi-unit Aesthetic

## Anti-rotational prosthetics

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. Indicated for unitary screw-retained prostheses.



### Multi-unit Aesthetic narrow straight abutment

1 mm	Ref. MUSA S04010
2 mm	Ref. MUSA S04020
3 mm	Ref. MUSA S04030
4 mm	Ref. MUSA S04040
5 mm	Ref. MUSA S04050



### Multi-unit Aesthetic slim straight abutment

2 mm	Ref. MUSLA 04020
3 mm	Ref. MUSLA 04030
4 mm	Ref. MUSLA 04040
5 mm	Ref. MUSLA 04050

C€0051

### Healing cap



Ref. PCT 4030



Ref. PCT 4830

### Temporary abutment



Ref. PTIMUA 4048

C€0051

### Impression technique

#### IMPRESSION COPING



Ref. AIPT 40

#### SCAN-BODY



Ref. SBT MUSA

#### IMPRESSION SCREW



Ref. TAIP 135



Ref. TAIP 200

Laboratory use only

#### ANALOG



Ref. RIT SB 40



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

C€

### Interfaces

The interfaces can be acquired in package that contains an interface and two **TMU 4048** screws, one clinical and the other for the laboratory.



Ref. PGZMUA 4040



Ref. PCERCMUA 4040



Ref. PITEMUA DA4075



Ref. TMU 4048



Ref. TPIA DP4048

C€0051





# Transepithelial Multi-unit

## Straight and Angled Abutments

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placements is **30 Ncm**. Indicated for multiple screw-retained prostheses with high aesthetic requirements in posterior region.

### Angled Aesthetic Multi-unit abutment



3 mm (15°)	Ref. EMU 1504030
4 mm (15°)	Ref. EMU 1504040
5 mm (15°)	Ref. EMU 1504050
3 mm (30°)	Ref. EMU 3004030
4 mm (30°)	Ref. EMU 3004040
5 mm (30°)	Ref. EMU 3004050
5 mm (45°)	Ref. EMU 4504050
5 mm (50°)	Ref. EMU 5004050
5 mm (60°)	Ref. EMU 6004050



### Straight Multi-unit abutment

1 mm	Ref. MUST 04010
2 mm	Ref. MUST 04020
3 mm	Ref. MUST 04030

#### Healing cap



Ref. PCM 4830

#### Temporary abutment



Ref. PTIMUTR 40

CE0051

#### Impression technique

Laboratory use only

#### ANALOG



Ref. RIMA SB 40



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

#### IMPRESSION COPING



Ref. AIPMU 40

#### SCAN-BODY



Ref. SBT MUST

#### IMPRESSION SCREW



Ref. TAIPMU 135

CE0051

#### Interfaces



Ref. PCMUTR 40



Ref. PITEMUTR 4040



Ref. TMUT 40

CE

The interfaces can be acquired in package that contains an interface and two TMUT 40 screws, one clinical and the other for the laboratory.

CE0051



# Direct to implant

## Fixed prosthetics - ASC abutment

Abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**.



### ASC abutment

- 2 mm Ref. PEA DP04020
- 3 mm Ref. PEA DP04030
- 4 mm Ref. PEA DP04040

C€0051

### Healing abutment



- 1 mm Ref. PCS 04010
- 2 mm Ref. PCS 04020
- 4 mm Ref. PCS 04040
- 6 mm Ref. PCS 04060



- 4 mm Ref. PCCS 04040
- 6 mm Ref. PCCS 04060

### Temporary abutment

#### ROTATIONAL



- 1 mm Ref. PCIR 040

#### ANTI-ROTATIONAL



- 1 mm Ref. PCIA 04010
- 2 mm Ref. PCIA 04020
- 3 mm Ref. PCIA 04030
- 4 mm Ref. PCIA 04040

C€0051

### Impression technique

Closed tray

#### IMPRESSION COPING



Ref. AIPC 040



Ref. AIP 040

Open tray

#### IMPRESSION COPING



Ref. TAIP 0135



Ref. TAIP 0200

#### SCAN-BODY



Ref. SBT 040

Laboratory use only

#### ANALOG



Ref. RI SB 040



Ref. TMU 4048

In case of 3D printed model, you must use this screw with the analog.

C€

### Screws



Ref. TP 040



Ref. TPEA DP040

C€0051





# Direct to implant

## Fixed prosthetics - Rotational / Anti-rotational abutments

Abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. It is indicated for single or multiple cemented prosthetics.



**Straight rotational abutment for cementation**

2 mm Ref. PR 04000



**Straight anti-rotation abutment for cementation**

0 mm Ref. PA 04000

1 mm Ref. PA 04010

3 mm Ref. PA 04030

5 mm Ref. PA 04050



**Angled abutment for cementation**

1 mm (15°) Ref. PA 0154010

3 mm (15°) Ref. PA 0154030

5 mm (15°) Ref. PA 0154050

1 mm (30°) Ref. PA 0304010

3 mm (30°) Ref. PA 0304030

5 mm (30°) Ref. PA 0304050



**Ti-base for cement-retained prosthetics**

1 mm Ref. PGZA 04010

2 mm Ref. PGZA 04020

3 mm Ref. PGZA 04030

4 mm Ref. PGZA 04040



**Ti-base for cement-retained prosthetics**

2 mm Ref. PGZA 040207

3 mm Ref. PGZA 040307

4 mm Ref. PGZA 040407

5 mm Ref. PGZA 040507



**Interface compatible with CEREC System**

2 mm Ref. PCERC 04020

3 mm Ref. PCERC 04030

4 mm Ref. PCERC 04040

CE0051

### Healing abutment



1 mm Ref. PCS 04010

2 mm Ref. PCS 04020

4 mm Ref. PCS 04040

6 mm Ref. PCS 04060



4 mm Ref. PCCS 04040

6 mm Ref. PCCS 04060

### Temporary abutment

#### ROTATIONAL



1 mm Ref. PCIR 040

#### ANTI-ROTATIONAL



1 mm Ref. PCIA 04010

2 mm Ref. PCIA 04020

3 mm Ref. PCIA 04030

4 mm Ref. PCIA 04040

CE0051

Laboratory use only

#### ANALOG



Ref. RI SB 040



Ref. TMU 4048

In case of 3D printed model, you must use this screw with the analog.

### Impression technique

Closed tray

#### IMPRESSION COPING



Ref. AIPC 040



Ref. AIP 040

Open tray

#### IMPRESSION COPING



Ref. TAIP 0135



Ref. TAIP 0200

#### SCAN-BODY



Ref. SBT 040

CE

### Screws



Ref. TP 040

CE0051



# Direct to implant

## Removable prosthesis

Abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. It is indicated for implant-retained or implant-supported prostheses. It allows you to correct the angulation of the implants at 10° (PKO) and 30° (PKB).



### Overdent abutment

0,8 mm	Ref. PKO 04008
1,6 mm	Ref. PKO 04016
3 mm	Ref. PKO 04030
4 mm	Ref. PKO 04040
5 mm	Ref. PKO 04050
7 mm	Ref. PKO 04070



### Ball abutment

0,8 mm	Ref. PKB 04008
1,6 mm	Ref. PKB 04016
3 mm	Ref. PKB 04030
4 mm	Ref. PKB 04040
5 mm	Ref. PKB 04050

CE0051

### Components for KO



Ref. TKO 4048



Ref. AKO 4048



Ref. RKO 4048



Ref. PKOC 08

### Components for KB



Ref. TKB 4048



Ref. AKO 4048



Ref. OB 4048

CE0051

### Impression technique

Closed tray

### IMPRESSION COPING



Ref. AIPC 040



Ref. AIP 040

Open tray

### IMPRESSION COPING



Ref. TAIP 0135



Ref. TAIP 0200

### SCAN-BODY




Ref. SBT 040

Laboratory use only

### ANALOG



Ref. RI SB 040



Ref. TMU 4048

In case of 3D printed model, you must use this screw with the analog

CE



# Tools



## Dual Screwdriver (LLDC 174, LLDC 220 y LLDL 290)

These wrenches have a double function, they serve both to give manual torque and to use with a ratchet. Available in 3 lengths: 17,4, 22 and 29 millimeters.

## ASC Dual Screwdriver (LLDP 220 y LLDP 290)

These wrenches have a double function, they serve both to give manual torque and to use with a ratchet for ASC. Available in 2 lengths: 22 and 29 millimeters.



## Manual Screwdriver (LLMC 220 y LLML 290)

These wrenches allow you to torque manually. With rotating crown and perforated for thread guides. Available in 2 lengths: 22 and 29 millimeters.

## Ultra short Screwdriver (LLCA 097)

This wrench allows you to give torque with the help of the ratchet.



## Overdent Screwdriver (LLKOD 250)

The square end allows the overdent abutment to be screwed and the opposite end allows the retention insert to be placed in the overdent cover.

## Multi-unit Screwdriver (LLCAMU 174 y LLCAMU 244)

They are used to place straight multi-unit with the help of the ratchet. Available in two lengths: 17,4 and 24,4 millimeters.



## Prosthetic Screwdriver (LLCAC 160 y LLCAC 250)

They connect to the manual screwdriver and are used to provide torque. Available in two lengths: 16 and 25 millimeters.

## Screwdriver direct from ratchet to implant (LLCAI 220 y LLCAI 290)

With the help of the ratched and connected directly to the internal connection of Galimplant implants, they allow their insertion. Available in two lengths: 22 and 29 millimeters.



## Direct motor Screwdriver (LLMI 295)

With the help of the motor and connected directly to the internal connection of the Galimplant implants, it allows their insertion.

## Prosthetic motor Screwdriver (LLMTP 220 y LLMTP 290)

These wrenches allow you to provide torque connected to the engine. Available in two lengths: 22 and 29 millimeters.



## Short, long and manual adapter (DC 144, DL 244 y DMA 150)


The short and long adapters are used to connect to the implant carrier and insert the implant with the help of the ratchet. The manual socket connected to the implant carrier is used to insert the implant manually.

## Motor Screwdriver (LLM 215)

Connected to the motor and the implant carrier, it allows the implant to be inserted.



“Committed to offering you solutions that provide **maximum aesthetics**, along with a **safe and predictable treatment**”

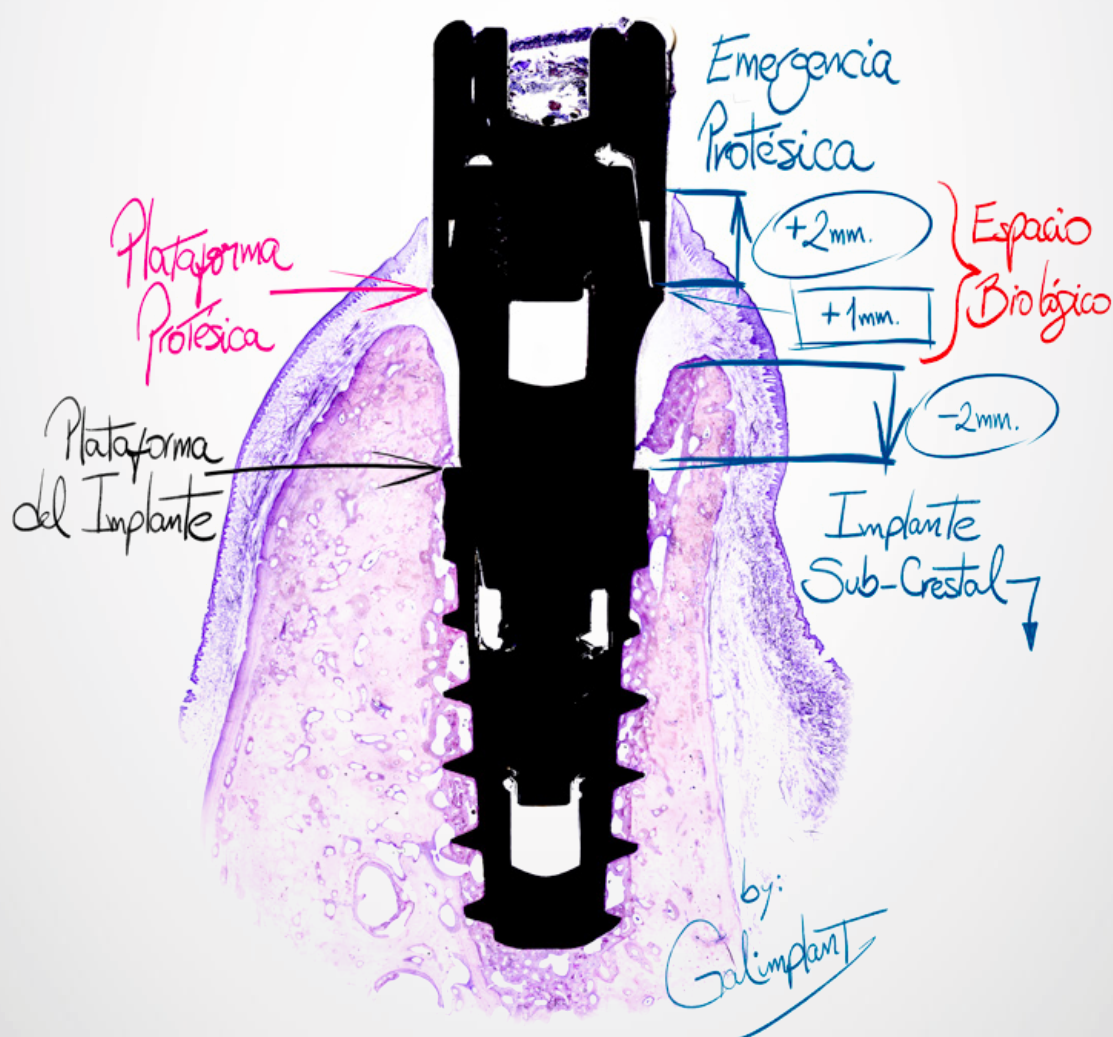

[www.galimplant.com](http://www.galimplant.com)



+34 982 533 493

C/Benigno Quiroga 90, 27600 - Sarria, Lugo (Spain)

CAT IPX-ICI - Vers. EN07/2024