



Implant system

IPX - ICI
Internal Connection



Just one **connection**, multiple **possibilities**

Galimplant Clásico System

Our dental implants are manufactured from **Grade IV Titanium**. They feature an **11° internal conical connection** and a **single prosthetic platform**. The **internal thread** of the **standard implants** is **1.6 mm**.



IPX

Macroscopic implant design that favors great primary stability in any situation.

		DIAMETER			
		Ø 3,5 mm	Ø 4 mm	Ø 4,5 mm	Ø 5 mm
LENGTH	6 mm	-----	Ref. IPX 4006S	Ref. IPX 4506S	Ref. IPX 5006S
	8 mm	Ref. IPX 3508S	Ref. IPX 4008S	Ref. IPX 4508S	Ref. IPX 5008S
	10 mm	Ref. IPX 3510S	Ref. IPX 4010S	Ref. IPX 4510S	Ref. IPX 5010S
	12 mm	Ref. IPX 3512S	Ref. IPX 4012S	Ref. IPX 4512S	Ref. IPX 5012S
	14 mm	Ref. IPX 3514S	Ref. IPX 4014S	Ref. IPX 4514S	-----
	16 mm	Ref. IPX 3516S	Ref. IPX 4016S	-----	-----
	18 mm	Ref. IPX 3518S	Ref. IPX 4018S	-----	-----

*If you want to select the closed-tray option, the order reference must include a 'C'. Example: **IPXC 3508S**

CE0051



ICI

Macroscopic implant design especially indicated for bone type I and II.

		DIAMETER			
		Ø 3,2 mm	Ø 3,5 mm	Ø 4 mm	Ø 5 mm
LENGTH	8 mm	-----	Ref. ICI 03508S	Ref. ICI 04008S	Ref. ICI 05008S
	10 mm	Ref. ICI 03210S	Ref. ICI 03510S	Ref. ICI 04010S	Ref. ICI 05010S
	12 mm	Ref. ICI 03212S	Ref. ICI 03512S	Ref. ICI 04012S	Ref. ICI 05012S
	14 mm	Ref. ICI 03214S	Ref. ICI 03514S	Ref. ICI 04014S	Ref. ICI 05014S

*If you want to select the closed-tray option, the order reference must include a 'C'. Example: **ICIC 03510S**

CE0051

Transepithelial Multi-unit Aesthetic

Multi-unit Prosthesis

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. Indicated for multiple screw-retained prostheses with high aesthetic demands.

Plataform 3,8 mm



Multi-unit Aesthetic narrow straight abutment

1 mm	Ref. MUSR 04010
2 mm	Ref. MUSR 04020
3 mm	Ref. MUSR 04030
4 mm	Ref. MUSR 04040
5 mm	Ref. MUSR 04050



Multi-unit Aesthetic slim straight abutment

2 mm	Ref. MUSLAR 04020
3 mm	Ref. MUSLAR 04030
4 mm	Ref. MUSLAR 04040
5 mm	Ref. MUSLAR 04050

CE0051

Healing abutment



Ref. EPCTR 4044



Ref. EPCTR 4844

CE0051

Impression technique

IMPRESSION COPING - SCREW



Ref. AIPTR 40



Ref. TAIP 135



Ref. TAIP 200

DIGITAL



Ref. SBT MUSR



Ref. TMU 4048

CE

Interfaces

The interfaces can be acquired in package that contains an interface and two **TMU 4048** screws, one clinical and the other for the laboratory.



Ref. PCERCUR 40



Ref. PITEMUR DA4075



Ref. PITEMUR DA4040



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

Laboratory use only

ANALOG



Ref. RITR SB 40



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

Transepithelial Multi-unit Aesthetic

Multi-unit Prosthesis

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placement is **30 Ncm**. Indicated for multiple screw-retained prostheses with high aesthetic requirements in posterior region.

Plataform 4,8 mm



Multi-unit Aesthetic wide straight abutment

- 2 mm Ref. MUSR 05020
- 3 mm Ref. MUSR 05030
- 4 mm Ref. MUSR 05040
- 5 mm Ref. MUSR 05050

Healing abutment



Ref. EPCTR 5044

CE0051

Impression technique

CE0051

IMPRESSION COPING - SCREW



Ref. AIPTR 50



Ref. TAIP 135



Ref. TAIP 200



Ref. SBT MUSR 50



Ref. TMU 4048

DIGITAL

Interfaces

CE



Ref. PITEMUR DA5075



Ref. PITEMUR DA5040



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

CE0051

Transepithelial Multi-unit Aesthetic

Single Crown Prosthesis

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placement is **35 Ncm**. Indicated for unitary screw-retained prostheses.

Plataform 3,8 mm



Multi-unit Aesthetic narrow straight abutment

- 1 mm Ref. MUSA S04010
- 2 mm Ref. MUSA S04020
- 3 mm Ref. MUSA S04030
- 4 mm Ref. MUSA S04040
- 5 mm Ref. MUSA S04050



Multi-unit Aesthetic slim straight abutment

- 2 mm Ref. MUSLA 04020
- 3 mm Ref. MUSLA 04030
- 4 mm Ref. MUSLA 04040
- 5 mm Ref. MUSLA 04050

Healing abutment



Ref. EPCTA 4844

CE0051

Impression technique

CE0051

IMPRESSION COPING - SCREW



Ref. AIPT 40



Ref. TAIP 135



Ref. TAIP 200



Ref. SBT MUSA



Ref. TMU 4048

DIGITAL

Interfaces

CE



Ref. PCERC MUA 40



Ref. PITEMUA DA4075



Ref. PITEMUA DA4040



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

CE0051

The interfaces can be acquired in package that contains an interface and two TMU 4048 screws, one clinical and the other for the laboratory.

Transepithelial Multi-unit

Straight and Angled Abutments

Transepithelial abutments made of **grade V titanium**. The **recommended torque** for its placements is **30 Ncm**. Indicated for multiple screw-retained prostheses with high aesthetic requirements in posterior region.

Angled Aesthetic Multi-unit abutment

3 mm (15°)	Ref. EMU 1504030
4 mm (15°)	Ref. EMU 1504040
5 mm (15°)	Ref. EMU 1504050
3 mm (30°)	Ref. EMU 3004030
4 mm (30°)	Ref. EMU 3004040
5 mm (30°)	Ref. EMU 3004050
5 mm (45°)	Ref. EMU 4504050
5 mm (50°)	Ref. EMU 5004050
5 mm (60°)	Ref. EMU 6004050

Straight Multi-unit abutment

1 mm	Ref. MUST 04010
2 mm	Ref. MUST 04020
3 mm	Ref. MUST 04030

Healing abutment



Ref. PCM 4830



Ref. TMUT 40

CE0051

Impression technique

IMPRESSION COPING - SCREW



Ref. AIPMU 40



Ref. TAIPMU 135

DIGITAL



Ref. SBT MUST



Ref. TMUT 40

Interfaces



Ref. PITEMUTR DA4040



Ref. PITEMUTR DA4075



Ref. TMUT 40

The **recommended insertion torque** is **10 Ncm**.

CE0051

CE

CE0051

Galimplant Único System

Our dental implants are manufactured from **Grade IV Titanium**. They feature an **11° internal conical connection** and a **single prosthetic platform**. The **internal thread** of the **uniqu implants** is **2.0 mm**, providing greater mechanical strength and structural robustness.

IPXC M2

Implant with a macroscopic design that promotes high primary stability in any situation. **2.0 Thread**.

DIAMETER

Ø 4 mm

Ø 4,5 mm

Ø 5 mm

LENGTH

8 mm	Ref. IPXC M2 4008S	Ref. IPXC M2 4508S	Ref. IPXC M2 5008S
10 mm	Ref. IPXC M2 4010S	Ref. IPXC M2 4510S	Ref. IPXC M2 5010S
12 mm	Ref. IPXC M2 4012S	Ref. IPXC M2 4512S	Ref. IPXC M2 5012S
14 mm	Ref. IPXC M2 4014S	Ref. IPXC M2 4514S	-----
16 mm	Ref. IPXC M2 4016S	-----	-----
18 mm	Ref. IPXC M2 4018S	-----	-----

CE0051

ICIC M2

Implant with a macroscopic design especially indicated for Type I and Type II bone. **2.0 Thread**.

DIAMETER

Ø 4 mm

Ø 5 mm

LENGTH

8 mm	Ref. ICIC M2 04008S	Ref. ICIC M2 05008S
10 mm	Ref. ICIC M2 04010S	Ref. ICIC M2 05010S
12 mm	Ref. ICIC M2 04012S	Ref. ICIC M2 05012S
14 mm	Ref. ICIC M2 04014S	Ref. ICIC M2 05014S

CE0051

Aesthetic Multi-position Trans-epithelial M2

Multi-unit Prosthesis

Trans-epithelial abutment made of **Grade V titanium**. The **recommended torque** for placement is **30 Ncm**.

Plataform 4,8 mm



Aesthetic straight multi-position M2 abutment

- 2 mm Ref. MUSR M2 05020
- 3 mm Ref. MUSR M2 05030
- 4 mm Ref. MUSR M2 05040
- 5 mm Ref. MUSR M2 05050

Healing abutment



Ref. EPCTR 5044

Impression technique

IMPRESSION COPING - SCREW



Ref. AIPT 50



Ref. TAIP 135



Ref. TAIP 200



Ref. SBT MUSR 50



Ref. TMU 4048

DIGITAL

ANALOG



Ref. RITR SB 50



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

Interfaces



Ref. PITEMUR DA5075



Ref. PITEMUR DA5040



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

CE0051

Aesthetic Multi-position Trans-epithelial M2

Single Crown Prosthesis

Trans-epithelial abutment made of **Grade V titanium**. The **recommended torque** for placement is **35 Ncm**.

Plataform 4,8 mm



Aesthetic straight multi-position M2 abutment

- 2 mm Ref. MUSA M2 S05020
- 3 mm Ref. MUSA M2 S05030
- 4 mm Ref. MUSA M2 S05040
- 5 mm Ref. MUSA M2 S05050

Healing abutment



Ref. EPCTA 5044

Impression technique

IMPRESSION COPING - SCREW



Ref. AIPT 50



Ref. TAIP 135



Ref. TAIP 200



Ref. SBT MUSA 50



Ref. TMU 4048

DIGITAL

ANALOG



Ref. RIT SB 50



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

Interfaces



Ref. PITEMUA DA5075



Ref. PITEMUA DA5040



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

CE0051

Trans-epithelial Multi-position M2

Convertible to external

Manufactured from **grade V titanium**. The **recommended insertion torque** is **30 Ncm**.

Plataform 3,8 mm



Multi-position abutment convertible to external M2

- 1 mm Ref. MUSTE M2 04010
- 2 mm Ref. MUSTE M2 04020
- 3 mm Ref. MUSTE M2 04030
- 4 mm Ref. MUSTE M2 04040

Healing abutment



Ref. EPCTER 4844



Ref. EPCTEA 4844

Multi-position abutment



Angled M2 Multi-position Abutment

- 15° Ref. CEMU 155040
- 30° Ref. CEMU 305045

CE0051

Impression technique

Laboratory use only

ANALOG



Ref. RI SB 40E



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

IMPRESSION COPING + SCREW



Ref. AIP 40T



Ref. TAIP 135

DIGITAL



Ref. SBT 40



Ref. TMU 4048

Interfaces

The interfaces can be acquired in package that contains an interface and two TMU 4048 screws, one clinical and the other for the laboratory.



Ref. PITEMUR DAE4075



Ref. PITEMUA DAE4075



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

CE0051

Impression technique

Laboratory use only

ANALOG



Ref. RITR SB 50



Ref. TRD

In case of 3D printed model, you must use this screw with the analog.

IMPRESSION COPING + SCREW



Ref. AIPTR 50



Ref. TAIP 135



Ref. TAIP 200

DIGITAL



Ref. SBT MUSR 50



Ref. TMU 4048

Interfaces

The interfaces can be acquired in package that contains an interface and two TMU 4048 screws, one clinical and the other for the laboratory.



Ref. PITEMUR DA5075



Ref. PITEMUR DA5040



Ref. TMU 4048

The recommended insertion torque is 30 Ncm.



Ref. TPIA DP4048

The recommended insertion torque is 15 Ncm.

CE0051

CE0051

Tools



Dual Screwdriver (LLDC 174, LLDC 220 y LLDL 290)

These wrenches have a double function, they serve both to give manual torque and to use with a ratchet. Available in 3 lengths: 17,4, 22 and 29 millimeters.

ASC Dual Screwdriver (LLDP 220 y LLDP 290)

These wrenches have a double function, they serve both to give manual torque and to use with a ratchet for ASC. Available in 2 lengths: 22 and 29 millimeters.



Manual Screwdriver (LLMC 220 y LLML 290)

These wrenches allow you to torque manually. With rotating crown and perforated for thread guides. Available in 2 lengths: 22 and 29 millimeters.

Ultra short Screwdriver (LLCA 097)

This wrench allows you to give torque with the help of the ratchet.



Overdent Screwdriver (LLKOD 250)

The square end allows the overdent abutment to be screwed and the opposite end allows the retention insert to be placed in the overdent cover.

Multi-unit Screwdriver (LLCAMU 174 y LLCAMU 244)

They are used to place straight multi-unit with the help of the ratchet. Available in two lengths: 17,4 and 24,4 millimeters.



Prosthetic Screwdriver (LLCAC 160 y LLCAC 250)

They connect to the manual screwdriver and are used to provide torque. Available in two lengths: 16 and 25 millimeters.

Screwdriver direct from ratchet to implant (LLCAI 220 y LLCAI 290)

With the help of the ratchet and connected directly to the internal connection of Galimplant implants, they allow their insertion. Available in two lengths: 22 and 29 millimeters.



Direct motor Screwdriver (LLMI 295)

With the help of the motor and connected directly to the internal connection of the Galimplant implants, it allows their insertion.

Prosthetic motor Screwdriver (LLMTP 220 y LLMTP 290)

These wrenches allow you to provide torque connected to the engine. Available in two lengths: 22 and 29 millimeters.



Short, long and manual adapter (DC 144, DL 244 y DMA 150)

The short and long adapters are used to connect to the implant carrier and insert the implant with the help of the ratchet. The manual socket connected to the implant carrier is used to insert the implant manually.


Motor Screwdriver (LLM 215)

Connected to the motor and the implant carrier, it allows the implant to be inserted.



CE

“Committed to offering you solutions that provide **maximum aesthetics**, along with a **safe and predictable treatment**”

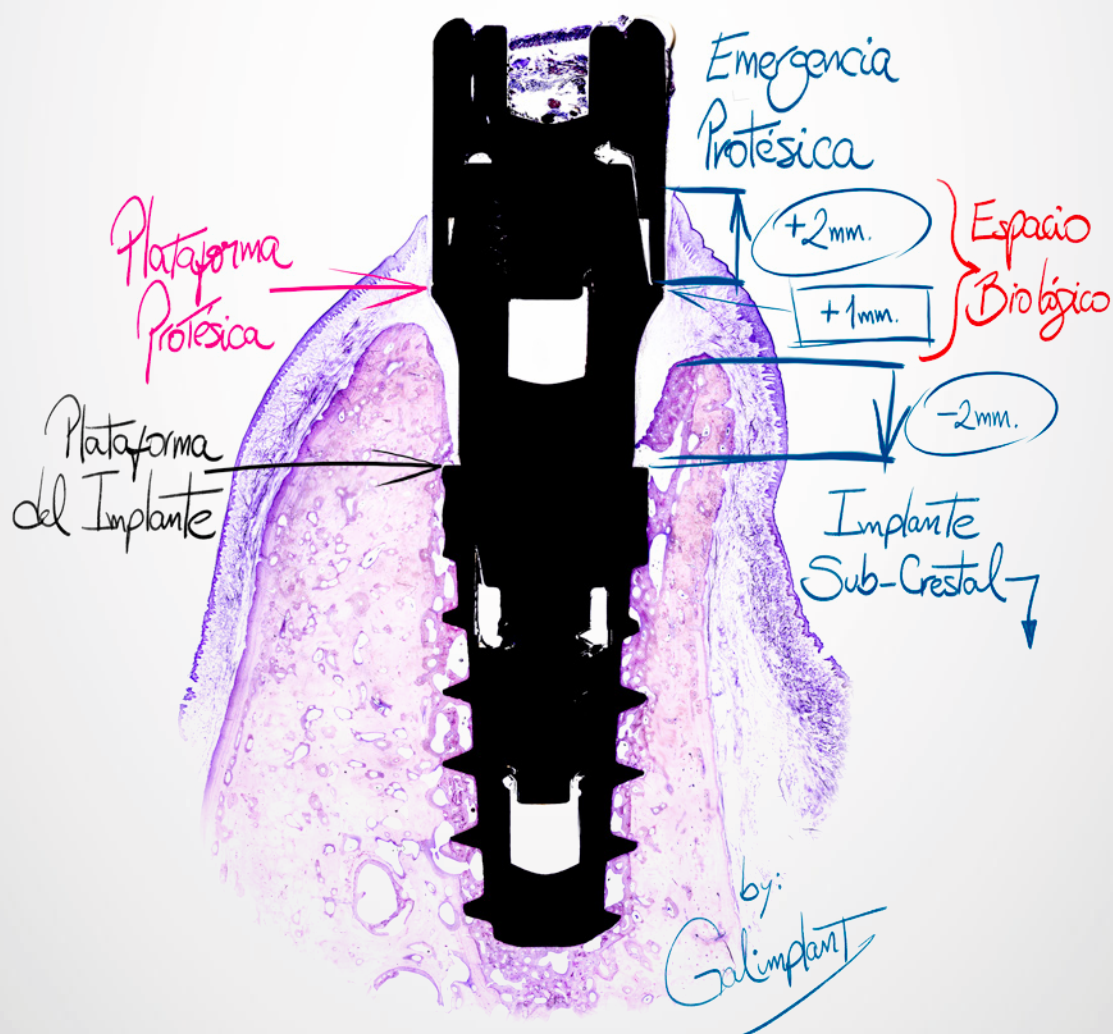

www.galimplant.com



+34 982 533 493

C/Benigno Quiroga 90, 27600 - Sarria, Lugo (Spain)